

ANALIZA BIAŁEK



100013826

Laboratory of Analysis

Client: PEPTOLOGY
Order number: 100013826
Name: PEPTOLOGY GLOW70
Number of samples: 1 vial

Batch number: PPT-GLW-070FX-0126
Receive date: 2026-04-08
Start date: 2026-04-16
End date: 2026-04-20

Sample identification

Substance	Method of taking a sample	Form
-----	Sample provided by customer	Purple powder in a glass vial

Results

Substance	Sample name	Content	Purity
BPC-157	PEPTOLOGY PEPTIDES GLOW70 70MG	10,67mg	99%
GHK-Cu	PEPTOLOGY PEPTIDES GLOW70 70MG	51,80mg	99%
TB-500	PEPTOLOGY PEPTIDES GLOW70 70MG	10,14mg	99%

Research comment

The test sample was applied in the amount of 3µl to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H2O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peaks of the sought substances appeared. Its concentration, when compared to the reference chromatogram shows the table above. Height the measurement error is + - 0,05 mg. The actual state of the sample sent before the test is presented on the photo below

Photo of the test sample




Password

CZ39GC16

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zajac




ANALIZA BIAŁEK




100013826

Chromatogram

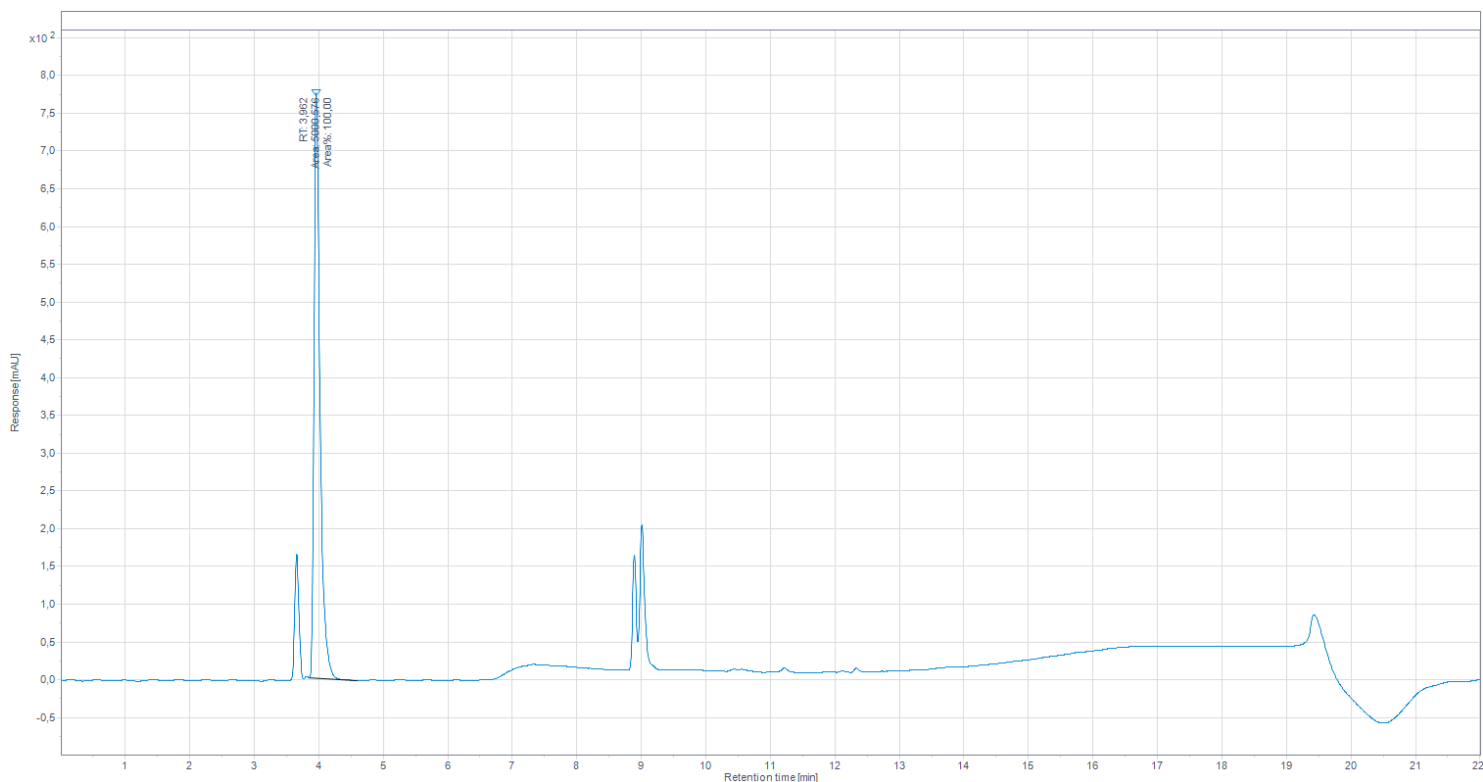

Chromatogram

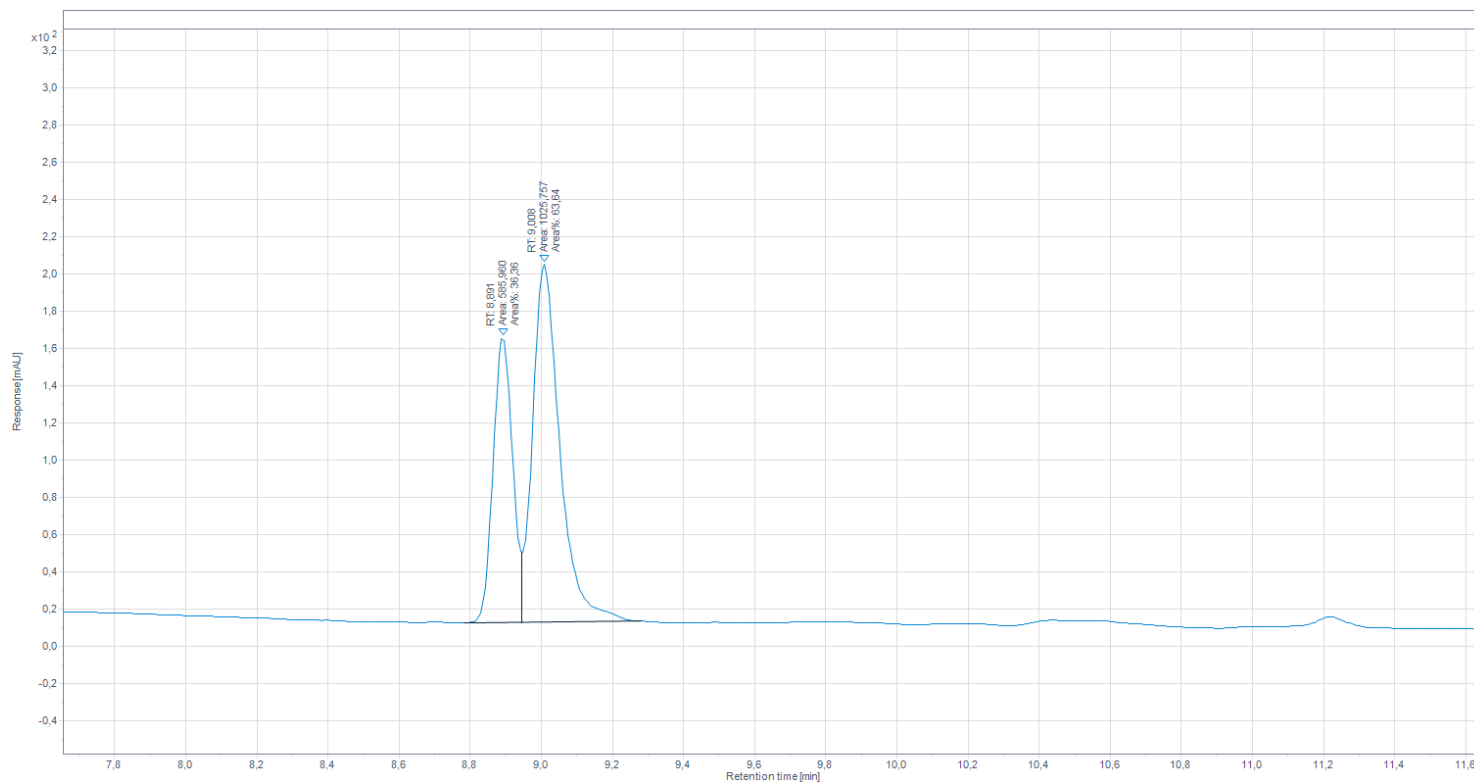

Password

CZ39GC16

Analiza Białek sp. z o.o.

KRS: 0000966168

NIP: 8992922970


REGON: 521751875

Headquarters and Laboratory:

ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:

Analysis and research specialist
mgr Arkadiusz Zajac



ANALIZA BIAŁEK



100013826

Method

Time	H ₂ O + 0,1% TFA	ACN + 0,1% TFA
0min	95%	5%
2min	95%	5%
12min	5%	95%
15min	5%	95%

Password

CZ39GC16

Analiza Białek sp. z o.o.

KRS: 0000966168

NIP: 8992922970

REGON: 521751875

Headquarters and Laboratory:

ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:

Analysis and research specialist
mgr Arkadiusz Zajac