

ANALIZA BIAŁEK



100016060

Laboratory of Analysis

Client: PEPTOLOGY
Order number: 100016060
Name: PEPTOLOGY KLOW80
Number of samples: 1 vial

Batch number: PPT-KLW-080FX-0226
Receive date: 2026-07-09
Start date: 2026-07-13
End date: 2026-07-23

Sample identification

Substance	Method of taking a sample	Form
-----	Sample provided by customer	Blue powder in a glass vial

Results

Substance	Sample name	Content	Purity
BPC-157	PEPTOLOGY KLOW80	10,60mg	99%
TB-500	PEPTOLOGY KLOW80	10,52mg	99%
GHK-Cu	PEPTOLOGY KLOW80	52,08mg	99%
KPV	PEPTOLOGY KLOW80	10,68mg	99%

Research comment

The test sample was applied in the amount of 3 μ l to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H₂O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peaks of the sought substances appeared. Its content, when compared to the reference chromatogram shows the table above. Height the measurement error is + - 0,05mg. The actual state of the sample sent before the test is presented on the photo below

Photo of the test sample




Password

CV89KM24

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zajac





ANALIZA BIAŁEK



100016060

Chromatogram

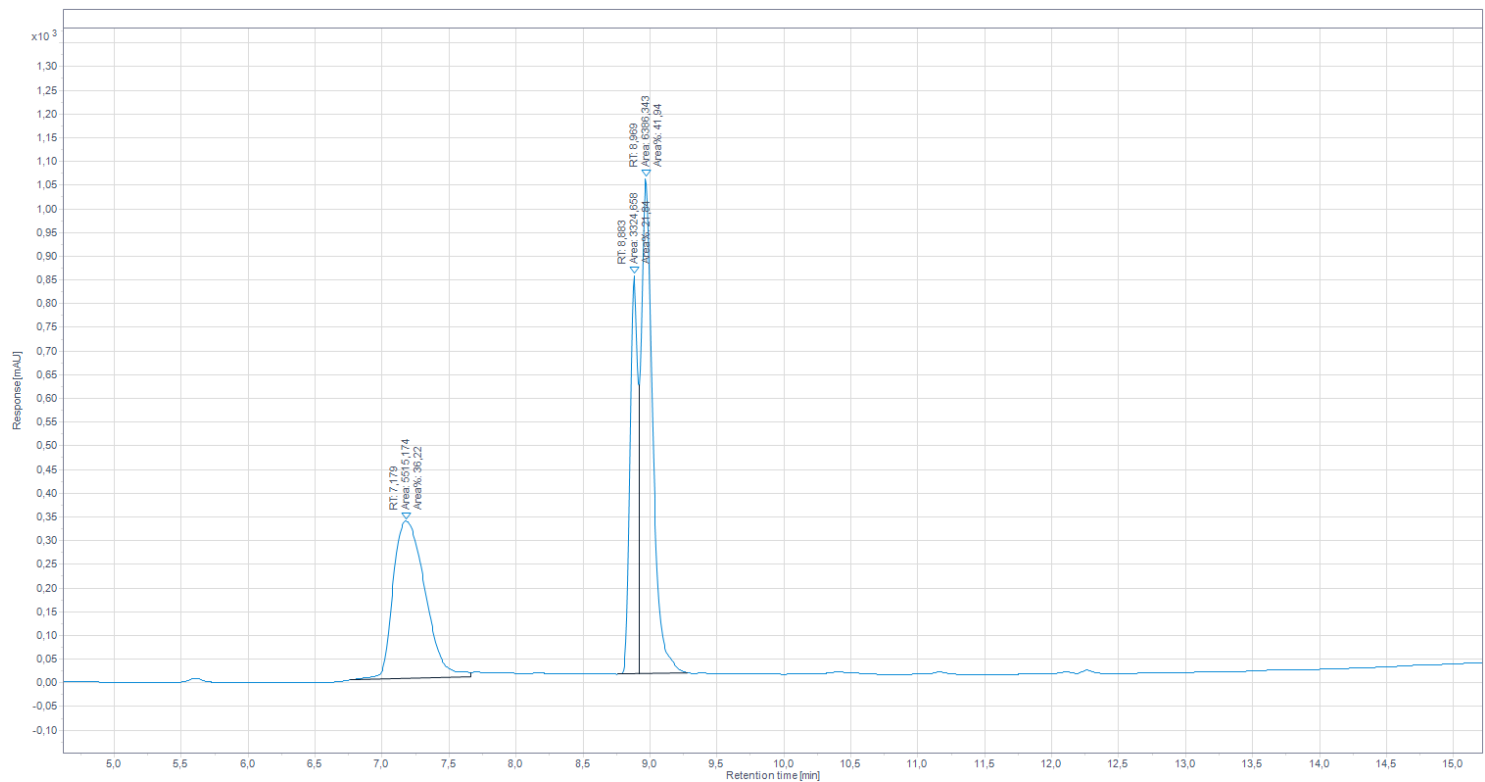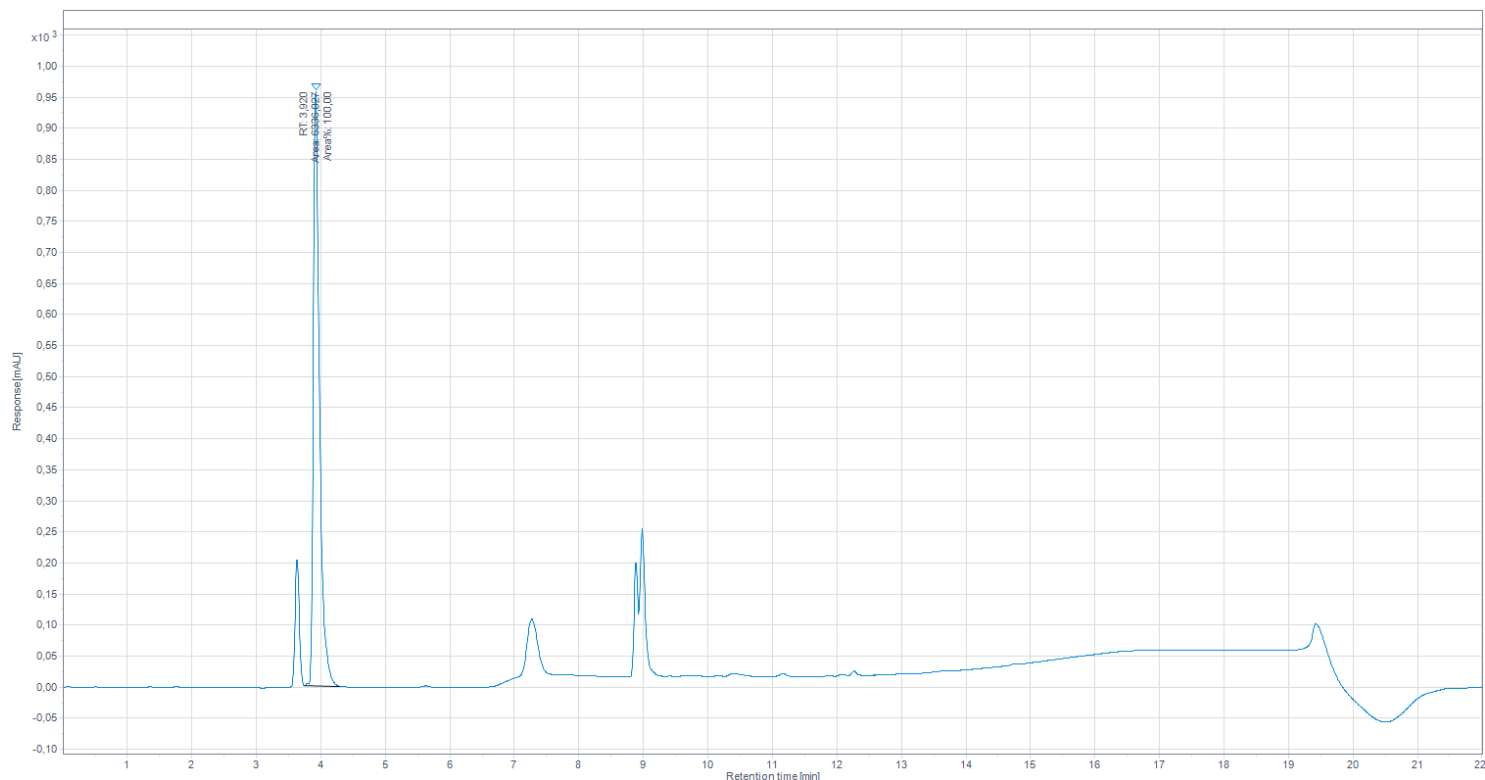

Password

CV89KM24

Analiza Białek sp. z o.o.

KRS: 0000966168

NIP: 8992922970


REGON: 521751875

Headquarters and Laboratory:

ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:

Analysis and research specialist
mgr Arkadiusz Zajac



ANALIZA BIAŁEK



100016060

Method

Time	H ₂ O + 0,1% TFA	ACN + 0,1% TFA
0min	95%	5%
2min	95%	5%
12min	5%	95%
15min	5%	95%

Password

CV89KM24

Analiza Białek sp. z o.o.

KRS: 0000966168

NIP: 8992922970

REGON: 521751875

Headquarters and Laboratory:

ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:

Analysis and research specialist
mgr Arkadiusz Zajac